

Administrative Data

Institution SZX
Physicist Krauss
PatientID zz-Leafspeed
Patient Name zz-Leafspeed, zz-Leafspeed
Comment TrueBeam Grün, Feber 2015

Data Set A

Q:_alle CHECKS\M1469\2015\02\Leafspeed\RI.zz-Leafspeed_R0.dcm

Data Set B

Q:_alle CHECKS\M1469\2015\02\Leafspeed\RI.zz-Leafspeed_RL.dcm

Manipulations

Command	Data Set	Parameters	Value
Region of interest	AB	Upper Left LR	-105.0 mm
		Upper Left TG	45.0 mm
		Lower Right LR	105.0 mm
		Lower Right TG	-45.0 mm


DoN (%Diff ref Norm. Value) - Parameters

Statistics

Number of Dose Points	123,280
Evaluated Dose Points	123,280 (100.0 %)
Passed	123,279 (100.0 %)
Failed	1 (0.0 %)
Result	100.0 % (Green)

Settings

Passing criteria	DoN \leq 3.0 %
Green	90.0 % to 100.0 %
Yellow	75.0 % to 90.0 %
Red	0.0 % to 75.0 %

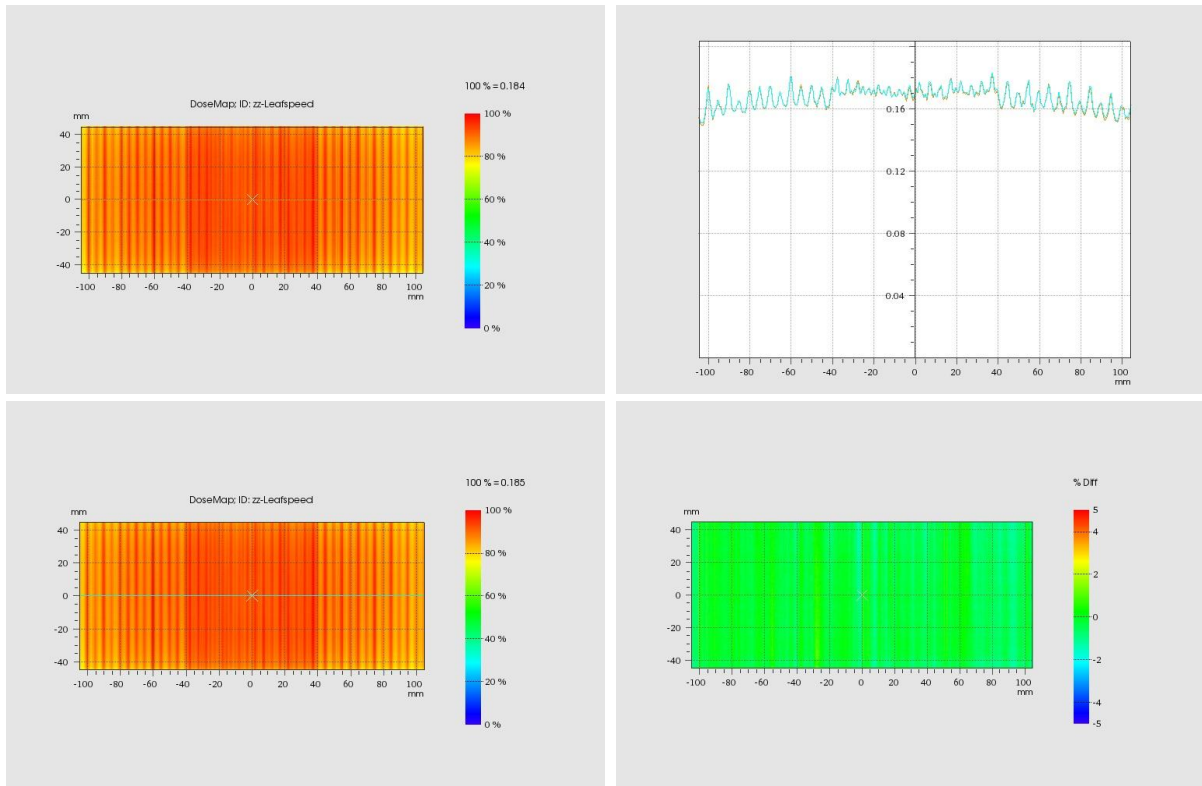

I hereby confirm that I have checked all data mentioned above and that the radiologic treatment according to this data shall / shall not proceed.

_____ Date

_____ Name and Function

_____ Signature